

ACCREDITED CALIBRATION, VERIFICATION SERVICE


Laboratory | Industry | Food Industry


PROFESSIONAL MEASURING





2025


KERN Pictograms


 **Internal adjusting**
Quick setting up of the balance's accuracy with internal adjusting weight (motordriven)


 **Adjusting program CAL**
For quick setting up of the balance's accuracy. External adjusting weight required


 **EasyTouch**
Suitable for the connection, data transmission and control through PC or tablet


 **Memory**
Balance memory capacity, e.g. for article data, weighing data, tare weights, PLU etc.


 **Alibi memory**
Secure, electronic archiving of weighing results, complying with the 2014/31/EU standard.


 **KERN Universal Port (KUP)**
allows the connection of external KUP interface adapters, e.g. RS-232, RS-485, SB, Bluetooth, WIFI, Analogue, Ethernet etc. for the exchange of data and control commands, without installation effort


 **RS-232 Data interface**
To connect the balance to a printer, PC or network


 **RS-485 Data interface**
To connect the balance to a printer, PC or other peripherals. Suitable for data transfer over large distances. Network in bus topology is possible


 **USB Data interface**
To connect the balance to a printer, PC or other peripherals


 **Bluetooth® Data interface**
To transfer data from the balance to a printer, PC or other peripherals

 **WIFI Data interface**
To transfer data from the balance to a printer, PC or other peripherals


 **Control outputs**
(optocoupler, digital I/O)
To connect relays, signal lamps, valves, etc.


 **Analogue interface**
to connect a suitable peripheral device for analogue processing of the measurements


 **Interface for second balance**
For direct connection of a second balance


 **Network interface**
For connecting the scale to an Ethernet network


 **KERN Communication Protocol (KCP)**
It is a standardized interface command set for KERN balances and other instruments, which allows retrieving and controlling all relevant parameters and functions of the device. KERN devices featuring KCP are thus easily integrated with computers, industrial controllers and other digital systems


 **GLP/ISO log intern**
The balance displays weight, date and time, independent of a printer connection


 **GLP/ISO log Printer**
With weight, date and time. Only with KERN printers.


 **Piece counting**
Reference quantities selectable. Display can be switched from piece to weight


 **Recipe level A**
The weights of the recipe ingredients can be added together and the total weight of the recipe can be printed out


 **Recipe level B**
Internal memory for complete recipes with name and target value of the recipe ingredients. User guidance through display


 **Totalising level A**
The weights of similar items can be added together and the total can be printed out


 **Percentage determination**
Determining the deviation in % from the target value (100 %)


 **Weighing units**
Can be switched to e.g. nonmetric units. See balance model. Please refer to KERN's website for more details

 **Weighing with tolerance range (Checkweighing)**
Upper and lower limiting can be programmed individually, e.g. for sorting and dosing. The process is supported by an audible or visual signal, see the relevant model


 **Hold function**
(Animal weighing program)
When the weighing conditions are unstable, a stable weight is calculated as an average value


 **Protection against dust and water splashes IPxx**
The type of protection is shown in the pictogram


 **Suspended weighing**
Load support with hook on the underside of the balance


 **Battery operation**
Ready for battery operation. The battery type is specified for each device


 **Rechargeable battery pack**
Rechargeable set


 **Universal plug-in power supply**
with universal input and optional input socket adapters for
A) EU, CH, GB
B) EU, CH, GB, US
C) EU, CH, GB, US, AUS


 **Plug-in power supply**
230V/50Hz in standard version for EU, CH. On request GB, USA or AUS version available


 **Integrated power supply unit**
Integrated in balance. 230V/50Hz standard EU. More standards e.g. GB, USA or AUS on request


 **Weighing principle Strain gauges**
Electrical resistor on an elastic deforming body


 **Weighing principle Tuning fork**
A resonating body is electromagnetically excited, causing it to oscillate


 **Weighing principle Electromagnetic force compensation**
Coil inside a permanent magnet. For the most accurate weighings


 **Weighing principle Single cell technology**
Advanced version of the force compensation principle with the highest level of precision

 **Conformity Assessment**
The time required for conformity assessment is specified in the pictogram

 **DAKkS calibration possible (DKD)**
The time required for DAKkS calibration is shown in days in the pictogram

 **Factory calibration (ISO)**
The time required for Factory calibration is shown in days in the pictogram

 **Package shipment**
The time required for internal shipping preparations is shown in days in the pictogram

 **Pallet shipment**
The time required for internal shipping preparations is shown in days in the pictogram

KERN Models A-Z

572	31
A	
ABP	50-51
ABP-A	52
ABT-NM	48
ACS / ACJ	46-47
ADB / ADJ	43
ADS / ADT <small>NEW</small>	49
ALS-A / ALJ-A	44-45
B	
BFC	120-121
BIC	117
BID	118-119
BXC <small>NEW</small>	122
C	
CB Q1 / CB Q2 / CB P1	156
CCA	90-91
CCS	92-93
CDS	89
CE Hx	134
CFS	86
CH	165
CIB	83
CJ P / CJ X	159
CKE	87
CO Y1 / CO Y2 / CO Y5	158
CP P4 / CP Y4 / CP P1 / CP Y1 / CP P3	153
CP P2 / CP P7 / CP P8	154
CR Q1 / CR P1 / CR Y1	155
CT Q1 / CT P1 / CT P2	157
CPB	85
CXB/CXB-NM	84
D	
DAB	54
DBS	55
DE	102-103
DLB	56
DS	111
E	
ECB-N / ECE-N	59
EFS	11
EHA	15
EMB	12
EMB-V	13
EMS	14
EOB	100
EOC	104-105
EOE	99
EOS	101
EW-N / EG-N	34
EWJ	30

F	
FCB	61
FCE-N	60
FCF	67
FES / FEJ	40
FFN	72
FGE	66
FKB	62
FOB-LM	68
FOB-S / FOB-NS	69
FOB / FOB-NL	70
FXN / FXN-M	73
H	
HCB	167
HCD	169
HCN	168
HDB-N / HDB-XL	166
HFA	170
HFC	171
HFD	172-173
HFM	174
I	
IFB	110
IFC	108-109
IFS	88
IOC	106-107
IXC	112-113
K	
KBP-V20 IP65	148
KDP	135
KFA-V20	150
KFB-TM	145
KFC-TM	146
KFD-V20	149
KFD-V40 IP68	151
KFN-TM	145
KFP-V20 IP65	148
KFP-V20 IP67	149
KFP-V30	150
KFP-V40 IP68	151
KFS-TM	144
KFU-V20	150
KFU-V30	150
KGP	132
KIB-TM	145
KIP-V20M	149
KXC-TM	147
KXP-V20 IP65	148

N	
NFC <small>NEW</small>	129
NIB	128
NXC <small>NEW</small>	130
P	
PBJ / PBS	37
PCB	26-27
PCD	24
PCJ	28-29
PDS / PDT	38-39
PEJ / PES	36
PFB	25
PLJ / PLS	32
PNS / PNJ	33
PWS	35
R	
RIB	78
RPB	79
S	
SCD-4.0	179
SCD-4.0-PRO	180
SFB / SFB-H	76
SFE	114
SXC	74-75
T	
TGC	9
TGD	9
U	
UFA	123
UFC <small>NEW</small>	126
UIB	124
UID	125
UXC <small>NEW</small>	127
V	
VHB	161
W	
WTB	71
Y	
YKV	133
YRO-01 / -02 / -03	185



KERN Quick-Finder

How I quickly find the product I am looking for


Ahead of each product group allows you to base the search for a certain target group on weighing data you need such as readout, weighing capacity and main features for each model.

And it's as simple as that – find the product you want in 2 steps:

1. Go to the product group index on page 3
2. Pick the appropriate product group and find the product you want using the Quick-Finder

Balance & weight in the quality management system

Do you already use all the modules of the KERN precision package for maximum accuracy and reliability of your balance?

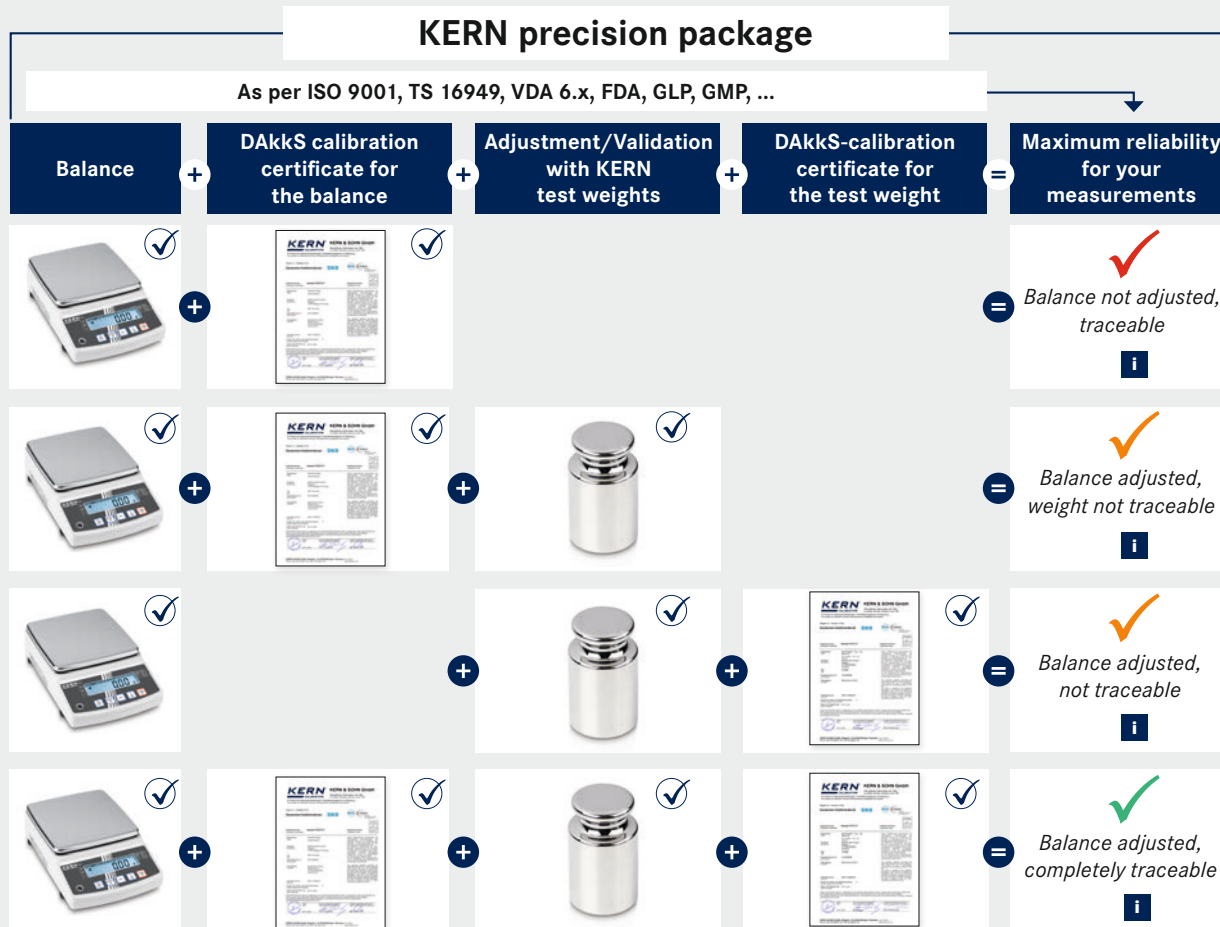

Information and ordering:
kern-sohn.com/qmb

The KERN calibration laboratory (D-K-19408-01-00)

KERN has a highly-automated DAkkS laboratory with accreditation to DIN EN ISO/IEC 17025 in numerous fields.

By using the most modern calibration technology with high-end calibration robots in fully air-conditioned laboratories, the measurement uncertainty and process times are reduced to a minimum, and also the quality of the calibration is increased.

As an accredited and certified calibration service provider with decades of experience, KERN offers you an extensive range of services, which will leave no demand unfulfilled. The accreditation applies to the extent specified in the appendix to the certificate D-K-19408-01-00.

We offer the following services:

Balances

- ▶ Accredited calibration up to 50 t
- ▶ Minimum sample weight (in use)
- ▶ Usage accuracy
- ▶ Adjustment at the location of installation
- ▶ Certificate of conformity
- ▶ Equipment qualification:
 - > Design qualification (DQ)
 - > Installation qualification (IQ)
 - > Function qualification (OQ)
 - > Performance qualification (PQ)
 - > Maintenance qualification (MQ)
- ▶ Conformity assessment/Verification

Weights

- ▶ Accredited calibration up to 2.5 t (OIML classes E1 – M3)
- ▶ Volume determination for OIML class E1
- ▶ Measuring of sensitivity (magnetic characteristics)
- ▶ Verification (where possible)

Force measuring devices and force transducers

- ▶ Accredited calibration up to 5 kN

Temperature and humidity sensors

- ▶ Accredited calibration up to 50 °C resp. 75 %

Factory calibration for

- ▶ Force measuring devices and force transducers ≤ 250 kN
- ▶ Hardness
- ▶ Layer thickness
- ▶ Material thickness
- ▶ Temperature of moisture analysers

Our commitment to satisfy our customers never stops. Perhaps this is one of the reasons why our roots can perhaps be traced so far back in history.
Discover the KERN route to success: fast – competent – reliable – versatile!

The order process

- 1** You will receive a **reminder** that your test equipment is due or you will generate online a quotation for new or existing test equipment
- 2** Submission or collection of your test equipment
- 3** Initial inspection of your goods, to check that they are suitable for calibration, and are complete, etc.
- 4** You will get a detailed **order confirmation**
- 5** Our experts will carry out **initial calibration**
- 6** Checked for conformity with required tolerances and if required, any **necessary actions** which arise from this are carried out
- 7** Before these actions are carried out, we will contact you (in so far as no **individual processing** has been agreed with you beforehand)
- 8** After your **approval** the necessary actions will be implemented and the calibration will be completed
- 9** After that your **test equipment will be returned** to you without delay, together with the appropriate calibration certificates
- 10** We will **monitor your recalibration periods** and will send you a reminder about your next calibration, free of charge

Our service

► Reminder service

The continuous cyclic recalibration of your checking equipment is an integral part of the reliable management of test equipment. You can rely on us to support you, and we will remind you in time, free of charge, when the next recalibration is due. In addition, you have the option of managing your test equipment online by yourself (cf. **1**, **10**).

► Quote generator

You will be impressed by our price-to-performance ratio. Request a non-binding quotation or create it yourself to suit your specifications at www.kern-lab.com (cf. **1**).

► Collection service

We will be pleased to arrange a pick up by our forwarding agent the goods from your premises. You only need to tell us the weight and dimensions of your package and leave the rest to us (cf. **2**).

► Repair and reconditioning of balances and weights

KERN will get your weights back up to standard, regardless of the manufacturer. Whether it is adjustment, marking, sand blasting or lacquering – the aim here is compliance and long-term stability. Any repairs of balances and instruments which may be necessary can be carried out quickly and easily (cf. **5**, **6**).

► Individual processing

In order to avoid delays with future orders, we would be pleased to incorporate your individual requirements for future processing of such calibration results. Even for smaller issues such as the printing of calibration certificates (stapling, punching, double-sided) we can work to your requirements (cf. **8**).

► Express service and dispatch

If you need a particularly fast service, you can use your DAKS express service. You will receive your test equipment after only 2 days (cf. **9**).

www.kern-lab.com – the central portal for everything you need to know about the extensive KERN calibration services

On our website you will always find the latest news and useful information about testing and measuring devices, calibration, legal metrology and expansions to our range of services. You will also find numerous online services on the website.

Database supported management of test equipment

Information on your test equipment which has been calibrated by us is stored in our database. In this way it is possible to make trend calculations. You will therefore get an overview about the long-term stability and trend behaviour of your test equipment as well as the necessary recalibration period can easily be determined and specified.

Paperless documentation

So there is no administrative effort, we can handle all calibration documentation in a paperless process. From quotation, through to order confirmation, delivery note and invoice right up to calibration certificate, you will receive all documents by e-mail or you can retrieve them online. Would you prefer to receive your certificate or your invoice in paper form, for example? Of course this is not a problem either.

We will send you everything you require by post.

Calibration certificate download

By using our download service you can easily download your calibration certificates as soon as the calibration work is complete and you will have access to them at any time in the future. Simply create your user account on www.kern-lab.com and you will never have to look for your certificates again.



Accredited Calibration of Balances

Any balance will only give correct results if it is checked regularly, i.e. calibrated correctly and adjusted when required. A balance is only a reliable measuring and checking tool if it is calibrated and this calibration is documented. The issued calibration certificates with accreditation symbol are proof of the metrological traceability to national and international standards, as required by the DIN EN ISO 9000 and DIN EN ISO/IEC 17025 standards, amongst others. KERN recommends a recalibration period of one year. The standard does not give a defined recalibration period. KERN recommends that, with intensive (daily) use, you to recalibrate your balance every 6 months and at normal (weekly) use, every 12 months.

The advantages of using on-site calibration:

- + **Calibration on-site** at your premises in the field of use
- + **Minimisation of measurement uncertainty** and guarantee of process accuracy strictly according to guideline EURAMET cg-18
- + **No risk of damage** during transportation
- + **Low downtime**
- + **Direct and personal contact** with the service technician
- + **Cross-brand servicing**, basic inspection and adjustment by a specialist
- + You tell us **when you would like us to come**
- + **Device training** for qualified users



a) KERN on-site calibration (we visit you)

In Germany, KERN has a close-knit network of KERN DAKKS calibration laboratory employees, who can carry out on-site calibration of balances up to 50 tonnes.

This on-site testing service is metrologically recommended, as your balance is in its field of use and can be calibrated without any possible transportation problems.

Lower downtime and personal contact with our expert are the major benefits of this service.

Preparatory maintenance work by agreement. Prices for on-site calibration on request.

You tell us when you would like us to come, giving us details of the balances to be tested. Our on-site DAKKS calibration team will then get in touch with you immediately and will discuss the process with you at your premises – it's straight forward and professional.

This KERN calibration service is also independent of the brand.

Please feel free to contact us at Phone +49 7433 9933-400 or E-Mail: testservices-onsite@kern-sohn.com

The advantages of using in-house calibration:

- + **Short calibration time:** Test time in the laboratory is only four working days
- + **Competence:** Calibration laboratory, which complies with the highest standards in the area of metrology
- + **Independent management** of the recalibration calendar for your individual measuring instrument is possible
- + **Cross-brand service:** Measuring devices from any manufacturer can be calibrated independently
- + **Repair:** Any necessary repairs can be carried out immediately, if you wish



b) Calibration at the KERN factory (you send your balance to us)

Recommended for new devices and for balances which can be affordably transported, as then there is no need for us to travel to carry out the calibration on-site. Repairs can be carried out at the same time, quickly and in full.

The process would be as follows:

- Day 1: Send your balance to the KERN calibration laboratory in Balingen.
- Day 2 to 3: Evaluation and calibration of your balance by our specialists.
- Day 4: After positive validation, your balance is returned.

Please feel free to contact us at Phone +49 7433 9933-400 or E-Mail: recalibration-balances@kern-sohn.com

Minimum weight of sample (in use)

What is the lightest item you can weigh on your balance, while still achieving accurate and reliable weighing results? What exactly is the limit?

The KERN minimum sample weight protocol accounts for the established minimum sample weight of your balance and its location of installation and use with the relative measuring uncertainty. With various safety coefficients and required weighing accuracy (process accuracy), depending on standard or quality-related requirements on the balance being used.

The higher the selected safety coefficient, the higher the safety when using the balance in a particular process.

Typical perturbations when using the balance e.g. small fluctuations in temperature are taken into account. In easily predictable conditions in a professional environment of use, KERN recommends a safety coefficient of 3. For critical processes, a correspondingly higher factor should be selected. The minimum sample weight protocol contains a diagram as well as a table, from which you can ascertain the minimum sample weight for your balance, depending on the process.

Adjustment at the location of installation

Why?

Adjustment at the location of installation is necessary, as the measuring results of balances depend on the local gravitational force (gravitational acceleration) and therefore depend on the location of use. KERN can carry this out just before shipping at the factor, individually to suit the location of installation.

What are the advantages of carrying out adjustment at the location of installation?

- The balance gives reliable measurement results at the location of installation.
- No time-consuming on-site adjustment necessary.
- You do not need a Service Engineer or any additional weights.
- The balance is ready for immediate use.

Pricing table for adjustment at the location of installation

Weighing capacity	KERN	Price excl. of VAT ex works €
[Max] ≤ 5 kg	961-247	43,-
[Max] > 5 – 50 kg	961-248	52,-
[Max] > 50 – 350 kg	961-249	62,-
[Max] > 350 – 1500 kg	961-250	99,-
[Max] > 1500 – 2900 kg	961-251	131,-
[Max] > 2900 – 6000 kg	961-252	260,-
[Max] > 6000 – 12000 kg	961-253	300,-

For adjustment to the location of installation you need the value for gravitational acceleration at the location of installation, which KERN can calculate using the point of use. The procedure is suitable for balances with a resolution of <60,000 d. For higher resolutions we recommend a balance with an internal adjusting weight or adjustment with a calibrated adjusting weight at the location of installation.

Certificate of conformity

With a certificate of conformity you get a statement about whether the balance meets your defined requirements. In conjunction with a calibration certificate with accreditation symbol it serves as documented proof that the balance fulfils the required process demands. When doing this the process owner for the balance can select from different temperature specifications – depending on its individual requirements:

Conformity evaluation on the basis of the:	KERN	Price excl. of VAT ex works €
Usage accuracy*	relative	969-511
	absolute	969-512
Calibration results*	relative	969-513
	absolute	969-514
Measurements as manufacturer or customer specification	Foreign device	969-515
	Customer specifications	969-516
	KERN devices	969-517

relative = % / absolute = g *as attachment to the calibration certificate with accreditation symbol (Details see www.kern-lab.com)

Example for absolute customer tolerance (absolute)
(Item no. 969-511):

No.	Tare	Load	Display	Deviation	Uncertainty	Customer tolerance	Conformity ¹⁾
1	0 g	500 g	500,00 g	0,00 g	± 0,013 g	± 0,05 g	☑
2	0 g	1000 g	1000,00 g	0,00 g	± 0,015 g	± 0,05 g	☑
3	0 g	1500 g	1500,01 g	0,01 g	± 0,017 g	± 0,05 g	☑
4	0 g	2000 g	2000,01 g	0,01 g	± 0,020 g	± 0,10 g	☑
5	0 g	3000 g	3000,02 g	0,02 g	± 0,022 g	± 0,10 g	☑

¹⁾Evaluation criteria: |[Deviation]| + [extended measuring uncertainty] ≤ [tolerance]

Documented quality of your balances in the log book

Consistently high product quality requires the use of measuring and test equipment that provides comprehensible, consistent and reproducible results. Hence, quality management systems require that measuring and test equipment produces a detailed traceable description and documentation of calibration results and conformity statements. According to the guiding principle of GMP/GLP: "Work not documented is work not done."

Equipment qualification is documentary evidence that a equipment is suitable for the intended purpose and is working faultlessly. A balance log book as well as our EQS (Equipment Qualification Software) is used to record all activities and results required for the qualification and monitoring of balances during routine operation. This includes the installation and commissioning of the balances, routine tests, maintenance as well as the recording of special events (failures, repairs, change of location).

The structure of the balance log book is based on the qualification process of the balance. The requirements for the qualification system such as DIN EN ISO 9001, DIN EN ISO/IEC 17025, GLP/GMP, VDA must be taken into account. The log book supports the user in his/her daily work with the balance and is meant to serve as necessary evidence during inspections and audits. The responsibility for maintaining the log book and its appropriate use is to be borne by the user.

Our proposal: Count on our support!

KERN offers this qualification concept throughout. Our validation services are carried out on the spot by technicians of our calibration laboratory and comprise among other things: installation, measurement test inclusive DAkks calibration certificate as well as records in your qualification log book of the EQS software (Equipment Qualification Software).

We give you advice about the options of device qualification, as required and will be happy to set up an appointment for qualification at the place of installation.

We offer individual calibration and maintenance agreements for the periodically required requalification.

Further information can be found at www.kern-lab.com



Important elements of equipment qualification:



Design qualification (DQ)

With the design qualification, which is carried out under consideration of a requirement specification/functional description, all the requirements on which you as a user depend on, are defined. The purchase decision is made on the basis of the design specifications and the available devices. Careful selection in the DQ can prevent subsequent deficiencies.



Installation qualification (IQ)

During the installation qualification based on a FMEA, we perform a documented installation, up to the qualified commissioning of your device. Points of this qualification are:

- Scope of delivery and identification
- Visual inspection of the system components
- Evaluation of the installation site
- Hardware installation and device settings
- Cleaning
- Query of work instructions during use
- Clarification of deviations
- Document review and approval

We carry out our qualifications in accordance with the GMP standard.



Function qualification (OQ)

Instruction is given to the user/s. Items of the OQ are:

- Function test of the system
- Initial adjustment on site
- Metrological verification including USP & Ph.Eur.
- Creation of test protocols
- Check of menu function and error message
- Review and approval of documents
- Evaluation of performance and determination of further test procedure



Performance qualification (PQ)

The PQ represents documented evidence that the balance or weighing system functions in the selected application as intended. This will be assured by a qualification test of the equipment under real conditions with respect to its surroundings and the problem definition (such as traceable data transmission).



Maintenance qualification (MQ)

The periodical maintenance, cleaning work and complete metrological test of the balance/weighing system is documented in the MQ by a trained authorised engineer. Maintenance is carried out with the help of a maintenance schedule. The maintenance times are determined by you. We are happy to support you with a maintenance contract for the entire organisation of your measuring system.



If you are interested in a training for equipment qualification, please feel free to contact us at **+49 7433 9933-400** or **testservices-onsite@kern-sohn.com**

KERN KERN & SOHN GmbH
 Akkreditiertes Kalibrierlabor seit 1994.
 Accredited calibration laboratory since 1994.

Ihr Partner für Kalibrierdienstleistungen, Prüfmittelmanagement und Beratung.
 Your partner for calibration services, test equipment management and support.

Mitglied im / member of the
Deutschen Kalibrierdienst **DKD** **DAKKS**

Sample
 D-K-19408-01-00
 2025-01

Kalibrierschein
 Calibration certificate

Sample-2025-01 **1**

Kalibrierzeichen
 Calibration mark

Gegenstand
 Object

Klasse E2

Gewichtssatz, 1 mg - 1 kg **2**

Hersteller
 Manufacturer

KERN & Sohn GmbH
 Zegelei 1
 D-72336 Balingen
 Germany

Type
 313-052 **3**

Fabrikat/Serien-Nr.
 Serial number

G123456789

Auftraggeber
 Customer

Mustermann GmbH **4**

Auftragsnummer
 Order No.

2023-123456789

Ort der Kalibrierung:
 Place of calibration

Kalibrierlaboratorium KERN
 Calibration - Laboratory KERN

Umgebungsbedingungen:
 Ambient conditions

Die Kalibrierung wurde bei folgenden Umgebungsbedingungen ausgeführt:
 The calibration was carried out under the following ambient conditions:

	von from	bis to	Unsicherheit uncertainty
Temperatur (°C) temperature	22,9	24,1	0,1
rel. Luftfeuchte (%) relative humidity	48,5	53,4	2,0
Luftdruck (hPa) air pressure	942,5	948,5	0,3

Magnetische Eigenschaften:
 Magnetic properties

Der Hersteller hat bestätigt, dass die Gewichtsstücke die magnetischen Eigenschaften gemäß R111:2004 einhalten.
 The manufacturer has confirmed the compliance of the magnetic properties of the weight pieces with the OIML R111:2004.

Referenzgewichte:
 Standard weights

123-D-K-19408-01-00-2025-05

Material / angenommene Dichte:
 Material / assumed density

Nennwert nominal value	Dichte density	Unsicherheit uncertainty	Material material	Form shape
1 mg - 500 mg	7950 kg/m³	140 kg/m³	Edelstahl Stainless steel	Draht Wire
1 g - 1 kg	8000 kg/m³	100 kg/m³	Edelstahl Stainless steel	Knopf Cylindrical form

Messergebnisse:
 Measurement results:

Nennwert nominal value	Kennzeichnung marking	konventioneller Wägewert conventional mass	Unsicherheit k=2 uncertainty	Fehlergrenze max. perm. error	Klasse* class*
1 mg		1 mg + 0.0010 mg	0.0020 mg	± 0.0060 mg	E2 ✓
2 mg		2 mg + 0.0005 mg	0.0020 mg	± 0.0060 mg	E2 ✓
2 mg	*	2 mg + 0.0016 mg	0.0020 mg	± 0.0060 mg	E2 ✓
5 mg		5 mg + 0.0010 mg	0.0020 mg	± 0.0060 mg	E2 ✓
10 mg		10 mg + 0.0009 mg	0.0020 mg	± 0.0060 mg	E2 ✓
20 mg		20 mg - 0.0001 mg	0.003 mg	± 0.010 mg	E2 ✓
20 mg	*	20 mg + 0.001 mg	0.003 mg	± 0.010 mg	E2 ✓
50 mg		50 mg + 0.001 mg	0.004 mg	± 0.012 mg	E2 ✓
100 mg		100 mg + 0.001 mg	0.005 mg	± 0.016 mg	E2 ✓
200 mg		200 mg + 0.002 mg	0.006 mg	± 0.020 mg	E2 ✓
200 mg	*	200 mg + 0.003 mg	0.006 mg	± 0.020 mg	E2 ✓
500 mg		500 mg + 0.005 mg	0.008 mg	± 0.025 mg	E2 ✓
1 g		1 g + 0.002 mg	0.010 mg	± 0.030 mg	E2 ✓
2 g		2 g + 0.002 mg	0.013 mg	± 0.040 mg	E2 ✓
2 g	*	2 g + 0.002 mg	0.013 mg	± 0.040 mg	E2 ✓
5 g		5 g + 0.010 mg	0.016 mg	± 0.050 mg	E2 ✓
10 g		10 g - 0.007 mg	0.020 mg	± 0.060 mg	E2 ✓
20 g		20 g + 0.005 mg	0.026 mg	± 0.080 mg	E2 ✓
20 g	*	20 g + 0.015 mg	0.026 mg	± 0.080 mg	E2 ✓
50 g		50 g + 0.02 mg	0.03 mg	± 0.10 mg	E2 ✓
100 g		100 g + 0.01 mg	0.05 mg	± 0.16 mg	E2 ✓
200 g		200 g + 0.05 mg	0.10 mg	± 0.30 mg	E2 ✓
200 g	*	200 g - 0.00 mg	0.10 mg	± 0.30 mg	E2 ✓
500 g		500 g + 0.10 mg	0.25 mg	± 0.80 mg	E2 ✓
1 kg		1 kg + 0.1 mg	0.5 mg	± 1.6 mg	E2 ✓

* Bewertung der Klasse bzw. der Fehlergrenze (wenn keine Klassenangabe vorhanden ist) bezieht sich nur auf den konventionellen Wägewert.
 The assessment of the class / the max. perm. error (if no class assessment is given) only refers to the conventional mass.

Fehler! Keine Dokumentvariable verfügbar. | Fehler! Keine Dokumentvariable verfügbar. |
 Fehler! Keine Dokumentvariable verfügbar. | Fehler! Keine Dokumentvariable verfügbar. |

Calibration certificate with accreditation symbol for test weights (extract).

For more details on our calibration service and other useful information, please see the internet at www.kern-lab.com

Traceable KERN test weights – Calibration of test weights

Calibrated measuring equipment requires calibrated checking equipment. For balances, these are calibrated test weights, also called “standard weights”.

KERN will calibrate your test weights

- In all classes with permissible error limits E1–M3 according to OIML R111:2004 in sizes 1 mg to 2500 kg
- With free nominal value
- Newton (N)
- Independent of design (special designs)

The advantages of using the KERN in-house calibration

You send your test weights to us.

- Excellent price performance ratio
- The quickest processing time
 - Standard service: 4 working days
 - Express service: 48 hrs (new weights)
- The most modern calibration methods with robot controlled comparators allow the most accurate calibration results and fastest throughput time
- KERN calibration certificates with accreditation symbol are internationally recognised
- A calibration service which is independent of the brand
- KERN also reconditions existing customer weights (e.g. cleaning or readjustment)
- On request, we can also provide a pick-up and collection service with our parcel service

The advantages of using the KERN on-site calibration

We visit you.

We would be pleased to visit you within Germany and carry out the calibration of your reference standards to OIML classes M1–M3, 10 kg–2500 kg with permissible error limits, using our mobile MACOS system. Minimized downtime of your checking equipment and direct contact with our expert are the major benefits of this service. Price on request.

Recalibration

- The recalibration schedule depends on the frequency of use, the conditions of use and the safety requirements
- In terms of standardisation, no particular recalibration interval is specified
- We would recommend that you recalibrate your test weights every six months if they are used intensively, and every 12 months with normal use
- We would be pleased to monitor your recalibration schedule

- 1 Official document
- 2 Item to be calibrated
- 3 Traceability, see the *Glossary*
- 4 Identification/Applicant
- 5 Environmental conditions
- 6 Metrological component
- 7 Conventional mass
- 8 Uncertainty of measurement, see the *Glossary*

Class acc.	➔	E1 ²⁾ with volume determination		E1 ¹⁾ without volume determination		E2 ¹⁾		F1/F2 ¹⁾ * F2 only		M1/M2/M3 ¹⁾	
Nominal value	↓	KERN	Price € excl. of VAT ex works	KERN	Price € excl. of VAT ex works	KERN	Price € excl. of VAT ex works	KERN	Price € excl. of VAT ex works	KERN	Price € excl. of VAT ex works
1 mg	-	-	-	962-251R	82,-	962-351R	36,-	962-451R	23,-	962-651R	19,-
2 mg	-	-	-	962-252R	82,-	962-352R	36,-	962-452R	23,-	962-652R	19,-
5 mg	-	-	-	962-253R	82,-	962-353R	36,-	962-453R	23,-	962-653R	19,-
10 mg	-	-	-	962-254R	82,-	962-354R	36,-	962-454R	23,-	962-654R	19,-
20 mg	-	-	-	962-255R	82,-	962-355R	36,-	962-455R	23,-	962-655R	19,-
50 mg	-	-	-	962-256R	82,-	962-356R	36,-	962-456R	23,-	962-656R	19,-
100 mg	-	-	-	962-257R	82,-	962-357R	36,-	962-457R	23,-	962-657R	19,-
200 mg	-	-	-	962-258R	82,-	962-358R	36,-	962-458R	23,-	962-658R	19,-
500 mg	-	-	-	962-259R	82,-	962-359R	36,-	962-459R	23,-	962-659R	19,-
1 g	963-231	250,-	962-231R	82,-	962-331R	36,-	962-431R	23,-	962-631R	19,-	
2 g	963-232	250,-	962-232R	82,-	962-332R	36,-	962-432R	23,-	962-632R	19,-	
5 g	963-233	250,-	962-233R	82,-	962-333R	36,-	962-433R	23,-	962-633R	19,-	
10 g	963-234	250,-	962-234R	82,-	962-334R	36,-	962-434R	23,-	962-634R	19,-	
20 g	963-235	250,-	962-235R	82,-	962-335R	36,-	962-435R	23,-	962-635R	19,-	
50 g	963-236	250,-	962-236R	82,-	962-336R	36,-	962-436R	23,-	962-636R	19,-	
100 g	963-237	250,-	962-237R	82,-	962-337R	46,-	962-437R	26,-	962-637R	21,-	
200 g	963-238	250,-	962-238R	82,-	962-338R	46,-	962-438R	26,-	962-638R	21,-	
500 g	963-239	250,-	962-239R	82,-	962-339R	46,-	962-439R	26,-	962-639R	21,-	
1 kg	963-241	250,-	962-241R	82,-	962-341R	46,-	962-441R	26,-	962-641R	21,-	
2 kg	963-242	570,-	962-242R	101,-	962-342R	55,-	962-442R	33,-	962-642R	22,-	
5 kg	963-243	570,-	962-243R	101,-	962-343R	55,-	962-443R	33,-	962-643R	22,-	
10 kg	963-244	570,-	962-244R	101,-	962-344R	55,-	962-444R	33,-	962-644R	22,-	
20 kg	963-245	1320,-	962-245R	760,-	962-345R	72,-	962-445R	37,-	962-645R	29,-	
50 kg	963-246	1540,-	962-246R	840,-	962-346R	84,-	962-446R	51,-	962-646R	31,-	
100 kg	-	-	-	-	-	-	962-591R*	152,-	962-691R	82,-	
200 kg	-	-	-	-	-	-	962-592R*	152,-	962-692R	82,-	
500 kg	-	-	-	-	-	-	962-593R*	152,-	962-693R	82,-	
1000 kg	-	-	-	-	-	-	-	-	962-694R	179,-	
2000 kg	-	-	-	-	-	-	-	-	962-695R	330,-	
1 mg-500 mg	-	-	962-250R	530,-	962-350R	250,-	962-450R	131,-	962-650R	82,-	
1 mg-50 g	963-201	1440,-	962-201R	870,-	962-301R	410,-	962-401R	215,-	962-601R	140,-	
1 mg-100 g	963-202	1570,-	962-202R	900,-	962-302R	450,-	962-402R	235,-	962-602R	146,-	
1 mg-200 g	963-203	1800,-	962-203R	990,-	962-303R	510,-	962-403R	260,-	962-603R	164,-	
1 mg-500 g	963-204	1920,-	962-204R	1030,-	962-304R	550,-	962-404R	270,-	962-604R	172,-	
1 mg-1 kg	963-205	2040,-	962-205R	1110,-	962-305R	590,-	962-405R	285,-	962-605R	180,-	
1 mg-2 kg	963-206	2660,-	962-206R	1180,-	962-306R	650,-	962-406R	330,-	962-606R	198,-	
1 mg-5 kg	963-207	2980,-	962-207R	1230,-	962-307R	690,-	962-407R	345,-	962-607R	210,-	
1 mg-10 kg	963-208	3390,-	962-208R	1270,-	962-308R	740,-	962-408R	375,-	962-608R	215,-	
1 g-50 g	963-215	1040,-	962-215R	385,-	962-315R	169,-	962-415R	88,-	962-615R	54,-	
1 g-100 g	963-216	1130,-	962-216R	420,-	962-316R	200,-	962-416R	101,-	962-616R	65,-	
1 g-200 g	963-217	1380,-	962-217R	500,-	962-317R	265,-	962-417R	128,-	962-617R	80,-	
1 g-500 g	963-218	1500,-	962-218R	550,-	962-318R	305,-	962-418R	143,-	962-618R	90,-	
1 g-1 kg	963-219	1650,-	962-219R	590,-	962-319R	340,-	962-419R	157,-	962-619R	96,-	
1 g-2 kg	963-220	2310,-	962-220R	680,-	962-320R	420,-	962-420R	197,-	962-620R	117,-	
1 g-5 kg	963-221	2700,-	962-221R	700,-	962-321R	470,-	962-421R	215,-	962-621R	126,-	
1 g-10 kg	963-222	3150,-	962-222R	760,-	962-322R	510,-	962-422R	240,-	962-622R	136,-	

¹⁾ Processing time 4 working days, ²⁾ Processing time 15 working days, ¹⁾ Preparation of reverification of balances, 969-006R, € 26,-

Additional costs for preparation, overhaul and adjustment before the calibration	KERN	Price excl. of VAT ex works €
Preparation of weights (e.g. cleaning, etc.)		
Single weight	969-001R	5,-
Weight set	969-002R	21,-
Subsequent services are carried out after confirmation		
Continued overhaul of weights (e.g. wet-cleaning, markings, repair, special packaging, adjustment E1 (DAkkS only), E2 ...)	969-005R	T & M basis
Adjustment, per weight only available for weights with adjustment chamber (F1- M3)	969-010R	15,-
Second calibration after adjustment or substitution, per weight		
Class E1	969-210R	63,-
Class E1 incl. volume determination	969-211R	230,-
Class E2	969-310R	30,-
Class F1/F2	969-410R	20,-
Class M1- M3	969-610R	16,-
Testing of magnetic properties according to OIML R111:2004, per weight	961-115R	16,-
Calibration of NON-OIML test weights, additional price per weight	-	8,-

KERN Standard Service Time* ¹	
Standard service Class E2 – M3	4 working days
Standard service Class E1, 1 mg – 500 mg, and recalibration 1 g – 10 kg with a known volume	10 working days
Class E1, ≥ 1 g, incl. volume determination (new weights)	15 working days

¹⁾ The delivery time for recalibrations can vary depending on the order situation as well as in case of queries, bottlenecks, etc.



Express service in 48 hours
except for class E1

- Urgent order is received at KERN by 12:00 noon at the latest
- Ready for shipping at KERN within two working days, at 12:00 noon
- Return by standard parcel service or express shipping (Costs and processing time on request)
- Additional cost for Express Service, for each test weight, KERN 962-115 € 21,-
- For Express shipping

Verification Prices for Test Weights and (Crane) Scales

Class acc. OIML R 111:2004	➔ E2 ¹⁾ with verification certificate	F1 ¹⁾ with verification certificate	M1 ¹⁾ with verification certificate			
Nominal value ↓	KERN	Price € excl. of VAT ex works	KERN	Price € excl. of VAT ex works	KERN	Price € excl. of VAT ex works
1 mg	952-351	57,-	952-451	48,-	952-651	34,-
2 mg	952-352	57,-	952-452	48,-	952-652	34,-
5 mg	952-353	57,-	952-453	48,-	952-653	34,-
10 mg	952-354	57,-	952-454	48,-	952-654	34,-
20 mg	952-355	57,-	952-455	48,-	952-655	34,-
50 mg	952-356	57,-	952-456	48,-	952-656	34,-
100 mg	952-357	57,-	952-457	48,-	952-657	34,-
200 mg	952-358	57,-	952-458	48,-	952-658	34,-
500 mg	952-359	57,-	952-459	48,-	952-659	34,-
1 g	952-331	57,-	952-431	48,-	952-631	34,-
2 g	952-332	57,-	952-432	48,-	952-632	34,-
5 g	952-333	57,-	952-433	48,-	952-633	34,-
10 g	952-334	57,-	952-434	48,-	952-634	34,-
20 g	952-335	57,-	952-435	48,-	952-635	34,-
50 g	952-336	57,-	952-436	48,-	952-636	34,-
100 g	952-337	63,-	952-437	48,-	952-637	34,-
200 g	952-338	63,-	952-438	50,-	952-638	34,-
500 g	952-339	63,-	952-439	50,-	952-639	34,-
1 kg	952-341	63,-	952-441	50,-	952-641	34,-
2 kg	952-342	71,-	952-442	57,-	952-642	36,-
5 kg	952-343	71,-	952-443	57,-	952-643	36,-
10 kg	952-344	71,-	952-444	57,-	952-644	44,-
20 kg	952-345	83,-	952-445	59,-	952-645	50,-
50 kg	-	-	952-446	70,-	952-646	52,-
1 mg-500 mg	952-350	285,-	952-450	148,-	952-650	92,-
1 mg-50 g	952-301	460,-	952-401	240,-	952-601	154,-
1 mg-100 g	952-302	500,-	952-402	260,-	952-602	164,-
1 mg-200 g	952-303	570,-	952-403	295,-	952-603	183,-
1 mg-500 g	952-304	610,-	952-404	305,-	952-604	192,-
1 mg-1 kg	952-305	630,-	952-405	320,-	952-605	200,-
1 mg-2 kg	952-306	720,-	952-406	360,-	952-606	220,-
1 mg-5 kg	952-307	790,-	952-407	395,-	952-607	235,-
1 mg-10 kg	952-308	830,-	952-408	420,-	952-608	240,-
1 g-50 g	952-315	185,-	952-415	107,-	952-615	70,-
1 g-100 g	952-316	220,-	952-416	113,-	952-616	75,-
1 g-200 g	952-317	290,-	952-417	145,-	952-617	89,-
1 g-500 g	952-318	330,-	952-418	160,-	952-618	99,-
1 g-1 kg	952-319	355,-	952-419	175,-	952-619	109,-
1 g-2 kg	952-320	445,-	952-420	220,-	952-620	130,-
1 g-5 kg	952-321	495,-	952-421	240,-	952-621	142,-
1 g-10 kg	952-322	550,-	952-422	270,-	952-622	152,-

KERN verification delivery time

Standard verification service Class E2 – M1	6 working days
--	----------------

Additional costs for preparation, overhaul and adjustment before the verification	KERN	Price excl. of VAT ex works €
--	------	--

Preparation of weights (e.g. cleaning, etc.)

Single weight	969-008R	5,-
Weight set	969-009R	21,-

Subsequent services are carried out after confirmation

Continued overhaul of weights (e.g. wet-cleaning, markings, repair, special packaging, adjustment E2 ...)	969-005R	T & M basis
--	----------	----------------

Adjustment, per weight only available for weights with adjustment chamber (F1/F2 – M1)	969-010R	15,-
---	----------	------

Verification after adjustment or substitution, per weight

Class E2	969-310R	30,-
Class F1/F2	969-410R	20,-
Class M1	969-610R	16,-

Verification prices for balances

Accuracy class I (precision balances) ¹⁾

[Max] ≤ 5 kg ¹⁾	950-101R	245,-
[Max] > 5 kg ¹⁾	950-102R	320,-

Accuracy class II (precision balances) ¹⁾

[Max] ≤ 5 kg ¹⁾	950-116R	126,-
[Max] > 5 kg – 50 kg ¹⁾	950-117R	153,-
[Max] > 50 kg – 350 kg ¹⁾	950-118R	235,-

Accuracy class III-IV ¹⁾

Bench scales and industrial scales (excl. crane scales)

[Max] ≤ 5 kg ¹⁾	950-127R	120,-
[Max] > 5 kg – 50 kg ¹⁾	950-128R	120,-
[Max] > 50 kg – 350 kg ¹⁾	950-129R	193,-
[Max] > 350 kg – 1500 kg ¹⁾	950-130R	285,-
[Max] > 1500 kg – 2900 kg ¹⁾	950-131R	395,-
[Max] > 2900 kg – 6000 kg ¹⁾	950-132R	610,-

Crane scales

[Max] > 50 kg – 350 kg ¹⁾	950-129HR	210,-
[Max] > 350 kg – 1500 kg ¹⁾	950-130HR	345,-
[Max] > 1500 kg – 2900 kg ¹⁾	950-131HR	500,-
[Max] > 2900 kg – 6000 kg ¹⁾	950-132HR	760,-
[Max] > 6000 kg – 12000 kg ¹⁾	950-133HR	1220,-


¹⁾ Preparation of reverification of balances, 969-006R, € 26,- ²⁾ Verification ("reverification") only in Germany

Our accreditation includes the calibration of tensile and pressure force up to 5 kN according to the standards DIN EN ISO 376 and DKD-R 3-3, each with the Newton (N) display unit for a complete measuring chain (situation A) or voltage ratio/transmission coefficient (mV/V, situation B).

Below you will find a comparison of which standard meets which criteria:

	ISO 376	DKD-R 3-3
Standardization	ISO standard (internationally standardized)	Standard of the DKD (Germany)
Measuring equipment	Force transducers and complete measuring chains	Force transducers and complete measuring chains
Area of application	Specifically force gauges for the testing of testing equipment	General force gauges
Number of power stages	8	5
Classification/Assessment	Classification in classes 00; 0,5; 1 and 2	None in standard
Test sequences	Fixed procedure	Sequences A, B, C, D possible Standard is sequence A B, C and D are reduced sequences, relevant previous knowledge is necessary
Summary	Higher-quality calibration, as 8 force levels are calibrated	High-quality calibration, reduced sequences with less effort possible

We can offer you a calibration solution for the following situations:

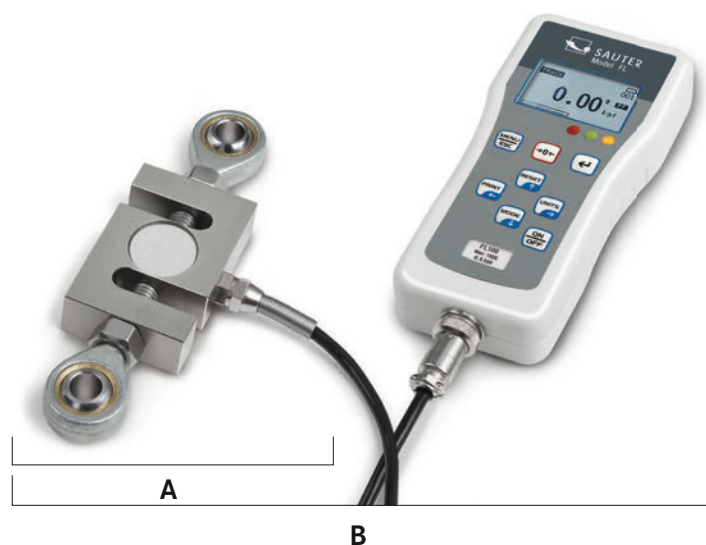

Situation A:
Separate force transducer,
display unit mV/V

Situation B:
Complete force gauge (N),
consisting of transducer, amplifier
and display, display unit N

► See also tables, right side



Prices for accredited calibration of force gauges and force transducers

Situation A: Force transducer (voltage ratio, in mV/V)* 1,2

ISO 376 (8 stages)			DKD-R 3-3 (5 stages, sequence A)		
KERN	Measuring range	Price € ex works excl. of VAT	KERN	Measuring range	Price € ex works excl. of VAT
Tensile force:					
963-161IV (R)	≤ 500 N	250,-	963-161V (R)	≤ 500 N	235,-
963-162IV (R)	≤ 2 kN	300,-	963-162V (R)	≤ 2 kN	280,-
963-163IV (R)	≤ 5 kN	390,-	963-163V (R)	≤ 5 kN	360,-
Compression force:					
963-261IV (R)	≤ 500 N	250,-	963-261V (R)	≤ 500 N	235,-
963-262IV (R)	≤ 2 kN	300,-	963-262V (R)	≤ 2 kN	280,-
963-263IV (R)	≤ 5 kN	390,-	963-263V (R)	≤ 5 kN	360,-
Tensile and Compression force:					
963-361IV (R)	≤ 500 N	420,-	963-361V (R)	≤ 500 N	390,-
963-362IV (R)	≤ 2 kN	500,-	963-362V (R)	≤ 2 kN	465,-
963-363IV (R)	≤ 5 kN	670,-	963-363V (R)	≤ 5 kN	610,-

Situation B: Complete force gauge (in N)* 2

ISO 376 (8 stages)			DKD-R 3-3 (5 stages, sequence A)		
KERN	Measuring range	Price € ex works excl. of VAT	KERN	Measuring range	Price € ex works excl. of VAT
Tensile force:					
963-161I (R)	≤ 500 N	205,-	963-161 (R)	≤ 500 N	187,-
963-162I (R)	≤ 2 kN	250,-	963-162 (R)	≤ 2 kN	225,-
963-163I (R)	≤ 5 kN	345,-	963-163 (R)	≤ 5 kN	315,-
Compression force:					
963-261I (R)	≤ 500 N	205,-	963-261 (R)	≤ 500 N	187,-
963-262I (R)	≤ 2 kN	250,-	963-262 (R)	≤ 2 kN	225,-
963-263I (R)	≤ 5 kN	345,-	963-263 (R)	≤ 5 kN	315,-
Tensile and Compression force:					
963-361I (R)	≤ 500 N	375,-	963-361 (R)	≤ 500 N	340,-
963-362I (R)	≤ 2 kN	460,-	963-362 (R)	≤ 2 kN	420,-
963-363I (R)	≤ 5 kN	620,-	963-363 (R)	≤ 5 kN	560,-

Factory calibration for force

This is not an accredited calibration (no proof of metrological traceability).

Situation A: Force transducer (voltage ratio, in mV/V)* 1,2

Situation B: Complete force gauge (in N)* 2

KERN	Measuring range	Price € ex works excl. of VAT	KERN	Measuring range	Price € ex works excl. of VAT
Tensile force:					
961-161V (R)	≤ 500 N	235,-	961-161 (R)	≤ 500 N	187,-
961-162V (R)	≤ 2 kN	280,-	961-162 (R)	≤ 2 kN	225,-
961-163V (R)	≤ 5 kN	360,-	961-163 (R)	≤ 5 kN	315,-
961-164V (R)	≤ 20 kN	460,-	961-164 (R)	≤ 20 kN	410,-
961-165V (R)	≤ 50 kN	460,-	961-165 (R)	≤ 50 kN	410,-
961-166V (R)	≤ 250 kN	495,-	961-166 (R)	≤ 250 kN	455,-
Compression force:					
961-261V (R)	≤ 500 N	235,-	961-261 (R)	≤ 500 N	187,-
961-262V (R)	≤ 2 kN	280,-	961-262 (R)	≤ 2 kN	225,-
961-263V (R)	≤ 5 kN	360,-	961-263 (R)	≤ 5 kN	315,-
961-264V (R)	≤ 20 kN	460,-	961-264 (R)	≤ 20 kN	410,-
961-265V (R)	≤ 50 kN	460,-	961-265 (R)	≤ 50 kN	410,-
961-266V (R)	≤ 250 kN	495,-	961-266 (R)	≤ 250 kN	455,-
Tensile and Compression force:					
961-361V (R)	≤ 500 N	390,-	961-361 (R)	≤ 500 N	340,-
961-362V (R)	≤ 2 kN	465,-	961-362 (R)	≤ 2 kN	420,-
961-363V (R)	≤ 5 kN	610,-	961-363 (R)	≤ 5 kN	560,-
961-364V (R)	≤ 20 kN	660,-	961-364 (R)	≤ 20 kN	610,-
961-365V (R)	≤ 50 kN	660,-	961-365 (R)	≤ 50 kN	610,-
961-366V (R)	≤ 250 kN	720,-	961-366 (R)	≤ 250 kN	670,-

(R): Recalibration

For each force gauge without interface or from other manufacturers we charge a surcharge of € 10,- for the additional effort.


*1 Compatibility with our amplifiers required

*2 Installation in our measuring equipment required

- Mechanical balances (spring balances, etc.)
- Force-measuring devices up to 250 kN
- Measuring devices for layer thickness 0 μm – 2000 μm
- Hardness testing devices in accordance with Leeb tests
- Ultrasonic material thickness testing device 25 mm – 300 mm

KERN	Measuring device	Measuring range	Price excl. of VAT ex works €
Factory calibration			
961-110	Coating thickness	≤ 2000 µm F or N	167,-
961-112	Coating thickness	≤ 2000 µm FN	235,-
961-113	Wall thickness (ultra sound)	≤ 300 mm (in stainless steel)	167,-
961-114	Wall thickness (Test blocks)	≤ 300 mm	208,-
961-170	Hardness comparison plate (Shore)	For sets up to 7 plates	132,-
961-131	Hardness tester (Leeb)	400 – 800 HLD	167,-
961-132	Hardness comparison plate (Leeb)	Hardness comparison plate (for Leeb durometer)	167,-
961-270	Hardness (UCI)	200 - 800 HV	360,-
961-150	Length	≤ 300 mm	167,-
961-190	Light	≤ 200000 lx	325,-
961-100	Mechanical balances/ spring balances	≤ 5 kg	99,-
961-101	Mechanical balances/ spring balances	> 5 – 50 kg	123,-
961-102	Mechanical balances/ spring balances	> 50 – 350 kg	146,-
961-103	Mechanical balances/ spring balances	> 350 – 1500 kg	225,-
961-102K	Digital dynamometer KERN MAP	≤ 130 kg	167,-
961-120 (R)	Torque wrench test devices	1 Nm - 200 Nm	235,-
964-305	Temperature calibration for moisture analyzer*		174,-
961-290	Refractometers		135,-
Additional services			
962-116	Express service with 48 hour delivery		52,-/ instrument

*For an overview of calibratable instruments and test services for further measuring sizes see www.kern-lab.com

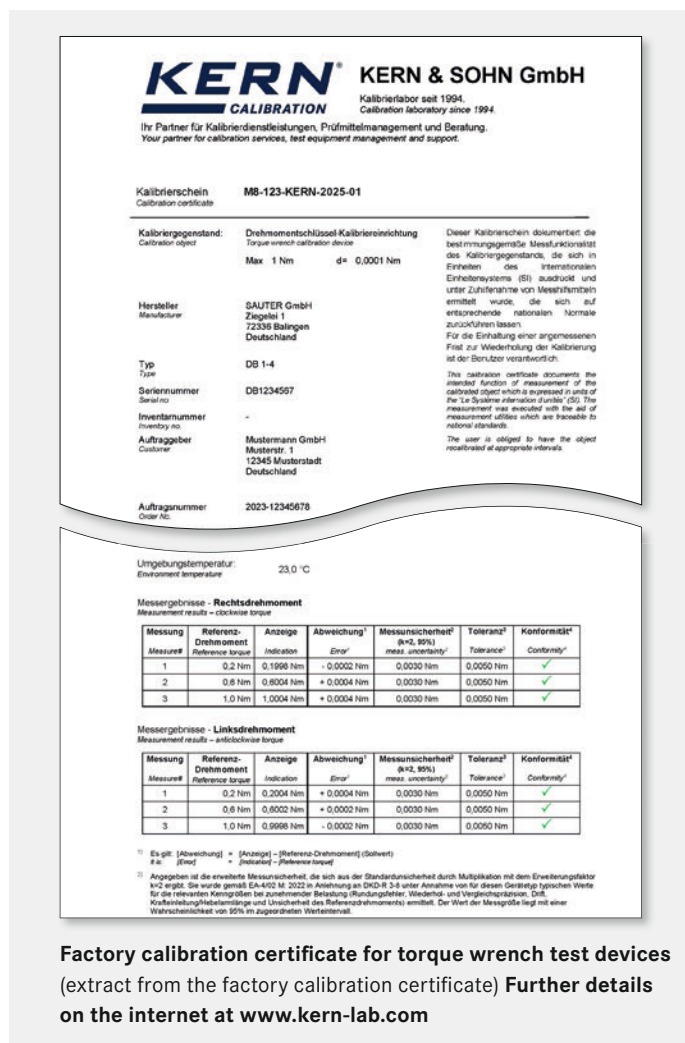

The oldest Precision Balance Factory in Germany

KERN & SOHN GmbH

Balances, Test Weights, Microscopes,
DAkkS Calibration Laboratory

Ziegelei 1
72336 Balingen
Germany
Tel. +49 7433 9933-0
info@kern-sohn.com
www.kern-sohn.com

Discover the multifaceted World of Balances, Microscopes and Measuring Technology from KERN online: www.kern-sohn.com

- Full KERN & SAUTER Product Range
- Convenient 24/7 Ordering
- Selection of more than 5,000 Items across Weighing and Measuring Technology, Optical Instruments as well as Accessories and Services
- Extensive Information and useful Download Options
- Technical Product Data Sheets
- Operating Instructions
- Descriptive Image and Video Material
- Useful KERN Services
- Technical Glossary
- KERN Dealer Portal
- Practical Filter and Search Functions



Follow us on our social media
channels too



Printed in Germany by KERN & SOHN GmbH
z-cb-en-kp-20251

